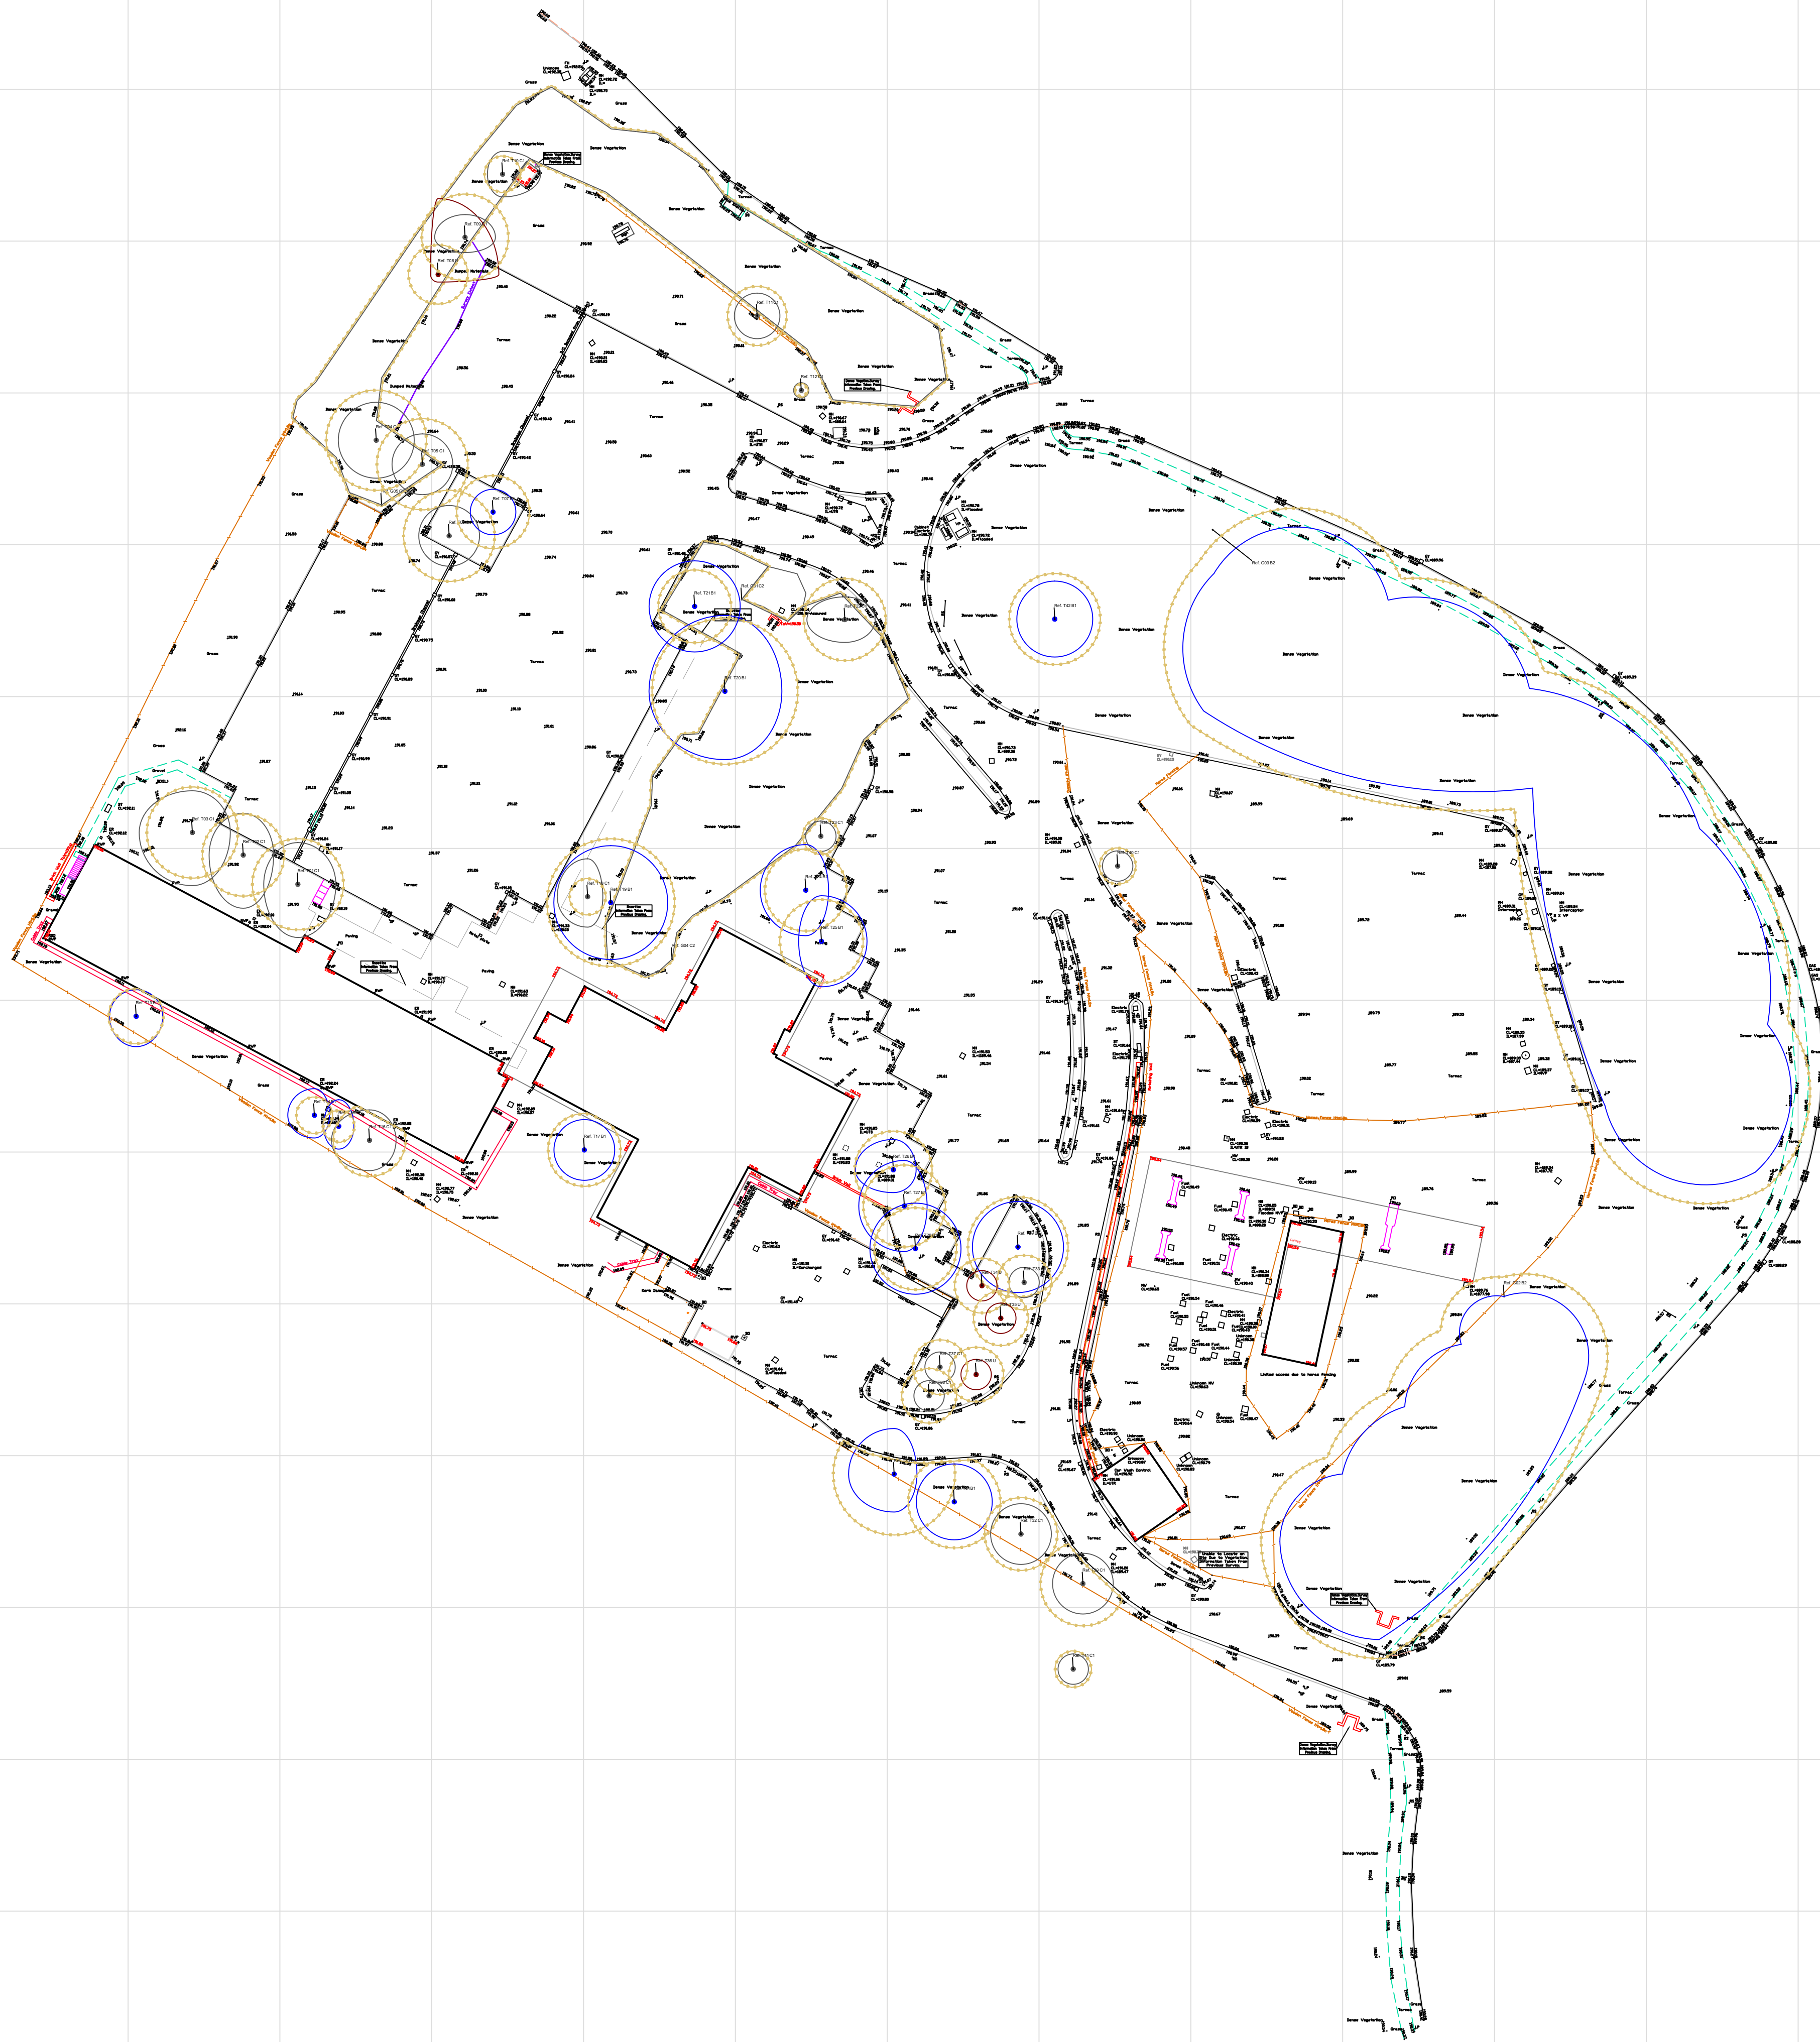


A1

This drawing has been prepared in accordance with BS 5837:2012.

This drawing is intended to be printed and used in colour only, and for no purpose other than the consideration of trees in accordance with BS 5837.

BS5837:2012 Cascade chart for tree quality assessment

Category & Definition	Criteria (including subcategories where appropriate)	Identification on plan
Tree quality assessment for retention:		
Category U	Upright trees with a canopy spread of less than 10m and a trunk diameter of less than 100mm. These trees are considered to be of low quality and are unlikely to be retained.	Red or Blue
Category A	Upright trees with a canopy spread of less than 10m and a trunk diameter of less than 100mm. These trees are considered to be of high quality and are likely to be retained.	Green
Category B	Upright trees with a canopy spread of less than 10m and a trunk diameter of less than 100mm. These trees are considered to be of medium quality and are likely to be retained.	Blue
Category C	Upright trees with a canopy spread of less than 10m and a trunk diameter of less than 100mm. These trees are considered to be of low quality and are unlikely to be retained.	Red or Blue

KEY

Root Protection Area (RPA)

Tree Stem

T1 Tree No.

Rev	Details	Date	Checked By

Drawing Number

AEL-19394

APEX

Apex Environmental Ltd

3 Lawrence Way, Lichfield, WS13 6RD

TEL. 0121 249 1235

e-mail. info@ael-treeconsultants.co.uk

web: www.ael-treeconsultants.co.uk

Client

EG on the move

Project

Travelodge Leicester Little Shaw Lane

Title

TCP-Tree Constraints Plan

Scale	Date	Drawn	Checked	Drawing No.	Rev
1:500	01/03/2016	RJH			A

This report is the copyright of Apex Environmental Ltd. Any unauthorised reproduction or usage by any person other than the addressee and LPA is strictly prohibited.